

# On the control of a muscular force model

AURORE MAILLARD  
Le2i CNRS UMR 6306  
Université de Bourgogne  
Franche-Comté, Arts et Métiers  
9 av. Alain Savary, 21000 Dijon  
FRANCE  
aurore.maillard@u-bourgogne.fr

TOUFIK BAKIR  
Le2i CNRS UMR 6306  
Université de Bourgogne  
Franche-Comté, Arts et Métiers  
9 av. Alain Savary, 21000 Dijon  
FRANCE  
toufik.bakir@u-bourgogne.fr

STÉPHANE BINCZAK  
Le2i CNRS UMR 6306  
Université de Bourgogne  
Franche-Comté, Arts et Métiers  
9 av. Alain Savary, 21000 Dijon  
FRANCE  
stbinc@u-bourgogne.fr

*Abstract:* Athletes and Physiotherapists may need electromyostimulation to reinforce muscle or to treat deficient muscles in order to speed up their recovery. Generally, the electromyostimulator does not take into account the physiological parameters necessary to adapt automatically the stimulation parameters of the system in order to reach a desired force value. To remedy at this problem and to optimize the rehabilitation sessions, we investigate the feasibility of controlling the muscular force by using an experimentally-based model.

*Key-Words:* Electrostimulation, Force muscular, Control

## 1 Introduction

Electromyostimulation is a process which arouses a lot of interest. As a consequence, this technique is often used for reinforcement and for reconditioning. Electromyostimulation (EMS) is carried out by placing electrodes on the area to be stimulated and electrical pulses are sent into the muscle to create involuntary contractions. The effects of these stimulations on the generated force are difficult to model. The modeling should be realized by mathematical models which take into account the physiological parameters, varying according to the subject state but also from one person to another, which renders the modeling difficult as explained in [1].

The model used in [2, 3] is obtained from experimental data and therefore satisfies specification requirements. Furthermore, it is based on a specific protocol which proves its reliability to solve the modeling problem of the relationship between force and stimulation accurately. Thus, this model could be used to maximize the force, which could be realized for instance by the prediction of the necessary number of muscular contractions. The predicted contraction frequency could also be used to analyze the correlation between the physiological aspects and the mathematical model [4]. The relationship between the force and the stimulation frequency can also be estimated on the same model, showing a correlation between the stimulation frequency and the effects on the force [5,6]. This model was tested in the case of children with cerebral paralysis (CP) in order to predict the obtained force level [7]. In this study, we based our

work on the model proposed in [2, 3], where the control variable acts on the impulse amplitude while the frequency is fixed. Section 2 details the equations of the model. Then in section 3, the nonlinear control strategy is proposed. In section 4, simulation results are presented, leading to quantify the control method efficiency. Finally, section 5 is devoted to the conclusion.

## 2 Model

The model used is defined by a set of differential equations, as follows:

$$\frac{dC_n}{dt} = \frac{1}{\tau_c} \sum_{i=1}^n R_i e^{-\frac{(t-t_i)}{\tau_c}} - \frac{C_n}{\tau_c}, \quad (1)$$

$$\frac{dF}{dt} = A \frac{C_n}{K_m + C_n} - \frac{F}{\tau_1 + \tau_2 \left( \frac{C_n}{K_m + C_n} \right)}, \quad (2)$$

with

$$R_i = 1 + (R_0 - 1)e^{-\frac{(t_i - t_{i-1})}{\tau_c}}. \quad (3)$$

Equation (1) represents the  $C_n$  derivative depending on  $C_n$  the normalized amount of  $C_a^{2+}$  - troponin complex obtained at each stimulation, the time constant  $\tau_c$  and the sum of successive pulses that are gathered in the term:

$$\sum_{i=1}^n R_i e^{-\frac{(t-t_i)}{\tau_c}}, \quad (4)$$

where  $t_i$  is the time of  $i^{th}$  pulse and  $R_i$  the mathematical term defining the magnitude of enhancement

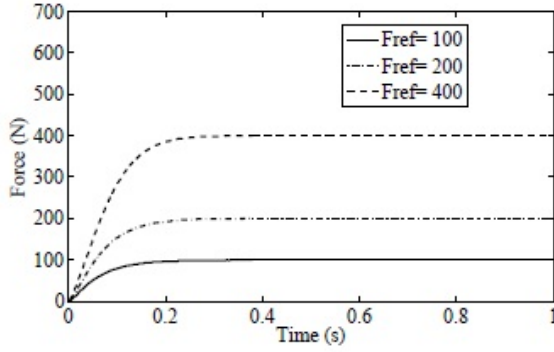


Figure 1: Evolution of the force value of control for  $F_{ref} = 100, 200$  and  $400$  N with  $dt = 10$  ms.

in  $C_n$  from the next stimuli.  $R_i$  is initialized at  $R_0$ . The stimulation generates a muscular force  $F$  according to (2). The parameters  $A$  (the scaling factor of the force and the muscle shortening velocity),  $R_0$  and  $\tau_1$  (a force time constant) are for this model at their resting values:  $A = 5.1$  N/ms,  $R_0 = 2$  and  $\tau_1 = 43.8$  ms and the parameters  $\tau_2 = 124.4$  ms,  $K_m = 0.3$  and  $\tau_c = 20$  ms, as defined in [2] with  $\tau_2$  the second force time constant and  $K_m$  the sensitivity of a strong bound crossbridges to  $C_n$ .

### 3 Control Method

The control method presented in this section is a nonlinear control applied to the force model. The variable  $u$  represents the control acting on the variation of impulse amplitudes. These amplitudes are found in the sum of exponential functions between two successive stimulations  $dt_i = t_{i+1} - t_i$ . The control is defined by the expression:

$$u = \frac{1}{\tau_c} \sum_{i=1}^n \alpha_i R_i e^{-\frac{(t-t_i)}{\tau_c}}, \quad (5)$$

so that (1) is modified as:

$$\frac{dC_n}{dt} = u - \frac{C_n}{\tau_c}. \quad (6)$$

Equation (5) includes a new parameter  $\alpha_i$  which is determined by the control  $u$ . Therefore, controlling the force corresponds to finding  $\alpha_i$  values. The control method is based on the prediction of the amplitude of the next pulse with  $dt_i$  constant. In the first part, we consider the case of a continuous control, named  $u_{NL}(t)$  then we deduct from it the discrete control  $u(t)$ , leading to determine  $\alpha_i$ .

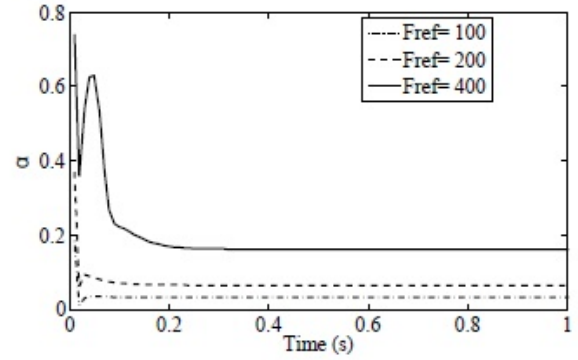


Figure 2: Evolution of the obtained impulse amplitude of control of the force for  $F_{ref} = 100, 200$  and  $400$  N with  $dt = 10$  ms.

In a general way, a nonlinear affine system function of  $u_{NL}(t)$  is described by the system (7), that is:

$$\dot{x}(t) = f(x(t)) + g(x(t))u_{NL}(t), \quad (7)$$

and

$$y(t) = h(x(t)). \quad (8)$$

According to the force model, one can write:

$$x(t) = \begin{bmatrix} C_n(t) \\ F(t) \end{bmatrix} = \begin{bmatrix} x_1(t) \\ x_2(t) \end{bmatrix}, \quad (9)$$

$$y(t) = x_2(t), \quad (10)$$

where  $f$  and  $g$  represent vector fields:

$$f = \begin{bmatrix} \frac{-x_1}{\tau_c} \\ \frac{Ax_1}{x_1 + K_m} - \frac{x_2}{\tau_1 + \tau_2 \frac{x_1}{x_1 + K_m}} \end{bmatrix} = \begin{bmatrix} f_1 \\ f_2 \end{bmatrix}, \quad (11)$$

$$g^T = [1 \ 0]^T. \quad (12)$$

Equation (10) expresses the fact that only the force  $F(t)$  is measured. Let us assume that the system is controllable, so that a control by output feedback would be possible. To perform this, we compute the first derivative of  $y(t)$ . From (7) and (8), it comes:

$$\dot{y}(t) = L_f h(x) + L_g h(x)u_{NL}(t), \quad (13)$$

where

$$L_f h(x) = \frac{\partial h}{\partial x} f, \quad (14)$$

$$L_g h(x) = \frac{\partial h}{\partial x} g. \quad (15)$$

It leads to:

$$L_f h(x) = [0 \ 1]f = f_2, \quad (16)$$

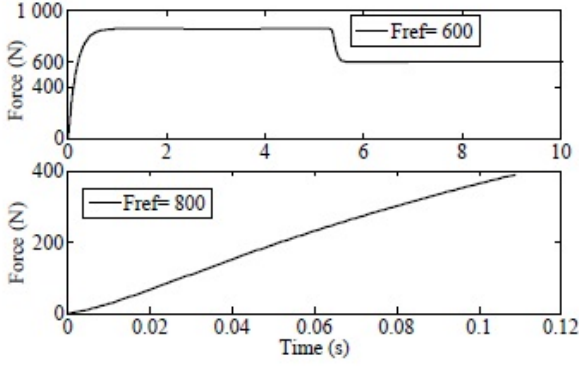


Figure 3: Representation of the generated forces for the control of the force for  $F_{ref}=600$  and  $800$  N with  $dt=10$  ms.

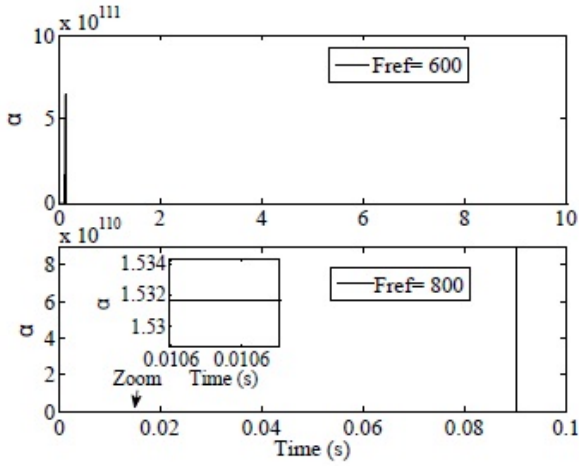


Figure 4: Evolution of the obtained impulse amplitude for the control of the force for  $F_{ref}=600$  and  $800$  N with  $dt=10$  ms.

$$L_g h(x) = [0 \ 1]g = 0. \quad (17)$$

As  $L_g h(x)$  is null, we compute the second derivative of  $y(t)$ . From (13), one can write:

$$\ddot{y}(t) = L_f^2 h(x) + L_g L_f h(x(t)) u_{NL}(t), \quad (18)$$

where

$$L_f^2 h(x) = L_f(L_f h(x)) = \frac{\partial L_f h(x)}{\partial x(t)} f, \quad (19)$$

and

$$L_g L_f h(x) = \frac{\partial L_f h(x)}{\partial x(t)} g = \left[ \frac{\partial L_f h(x)}{\partial x_1} \quad \frac{\partial L_f h(x)}{\partial x_2} \right] g. \quad (20)$$

So,

$$L_g L_f h(x) = \frac{AK_m}{(K_m + x_1)^2} + \frac{x_2 K_m \tau_2}{(\tau_1(K_m + x_1) + \tau_2 x_1)^2}. \quad (21)$$

From (21), one can verify that  $L_g L_f h(x)$  is  $\neq 0$ . Therefore, the nonlinear control  $u_{NL}(t)$  is defined such as:

$$u_{NL}(t) = \frac{-L_f^2 h(x) + v(t)}{L_g L_f h(x)}, \quad (22)$$

where  $\ddot{y}(t)$  has to be equal to  $v(t)$ , which is defined to stabilize the system to  $y_{ref}(t)$ , the target force. Let us assume that:

$$v(t) = \ddot{y}_{ref} - C_1(\dot{y}(t) - \dot{y}_{ref}(t)) - C_0(y(t) - y_{ref}(t)), \quad (23)$$

where  $C_1$  and  $C_0$  are constant parameters to be calculated in order to ensure stability system. Then,

$$\ddot{y}(t) = \ddot{y}_{ref}(t) - C_1(\dot{y}(t) - \dot{y}_{ref}(t)) - C_0(y(t) - y_{ref}(t)), \quad (24)$$

giving:

$$\ddot{y} - \ddot{y}_{ref} + C_1(\dot{y} - \dot{y}_{ref}) + C_0(y(t) - y_{ref}(t)) = 0. \quad (25)$$

Let us now define the error  $e(t)$  between the force  $y(t)$  and the target force  $y_{ref}(t)$ , that is :

$$e(t) = y(t) - y_{ref}(t). \quad (26)$$

Equation (25) becomes:

$$\ddot{e}(t) + C_1 \dot{e}(t) + C_0 e(t) = 0, \quad (27)$$

which corresponds to:

$$s^2 E(s) + C_1 s E(s) + C_0 E(s) = 0, \quad (28)$$

where  $E(s)$  is the Laplace transformation of  $e(t)$  and  $s$  the Laplace variable.  $e(t)$  tends to zero if  $s^2 + C_1 s + C_0 = 0$  is stable. The unknown parameters  $C_0$  and  $C_1$  are then chosen such that the roots of (28) have negative real parts (stable eigenvalues). A set of test has been performed using different couples  $(C_1, C_0)$  in order to choose acceptable tendency (overshoot, convergence speed) of the force evolution. For all the following, we used  $(C_1, C_0) = (-0.006, 0.05)$ . The nonlinear control ( $u_{NL}(t = ndt)$ ) being computed, it is used to compute the impulse amplitude to be applied at  $t$  (the real control  $u$  is a sum of successive impulses):

$$u = \frac{1}{\tau_c} \sum_{i=1}^n \alpha_i R_i e^{-\frac{(t-t_i)}{\tau_c}}. \quad (29)$$

To do that, we suppose that  $u_{NL}(t)$  is constant during the interval  $[t, t + dt[$  and chosen to be equal to the mean value of  $u(t)$  during the above interval. The effect of a control  $u$  will be approximately the same as

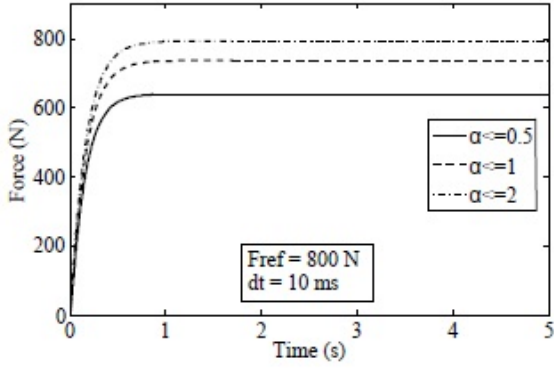


Figure 5: Different limits of impulse amplitudes for a  $F_{ref}$  of 800 N ( $dt=10$  ms).

$u_{NL}(t)$  which leads  $F$  to  $F_{ref}$ ,

$$u_{NL}(t) = \frac{1}{H+1} \sum_{k=0}^H u\left(t + \frac{k}{H}dt\right)$$

$$= \frac{1}{H+1} \sum_{k=0}^H \frac{1}{\tau_c} \sum_{i=1}^n R_i \alpha_i e^{-\frac{(t + \frac{k}{H}dt - t_i)}{\tau_c}}, \quad (30)$$

where  $H$  is the number of simulation values of  $u$  during  $[t, t+dt]$  equal to a chosen value fixed to 10 with the integration step  $\Delta T = \frac{dt}{H+1}$ . Therefore:

$$u_{NL}(t) = \frac{1}{H+1} \left[ \sum_{k=0}^H \frac{1}{\tau_c} \left[ \sum_{i=1}^{n-1} R_i \alpha_i e^{-\frac{(t + \frac{k}{H}dt - t_i)}{\tau_c}} + R_n \alpha_n e^{-\frac{(t + \frac{k}{H}dt - t_n)}{\tau_c}} \right] \right], \quad (31)$$

$\alpha_i$  ( $i = 1, \dots, n-1$ ) being the previous pulses amplitudes, which were computed using the previous stimulation steps. At time  $t = ndt$ , only the value of  $\alpha_n$  is unknown. From (31), it comes:

$$\alpha_n = \frac{(H+1)u_{NL}(t) - \sum_{k=0}^H \frac{1}{\tau_c} \left[ \sum_{i=1}^{n-1} R_i \alpha_i e^{-\frac{(t + \frac{k}{H}dt - t_i)}{\tau_c}} \right]}{\frac{R_n}{\tau_c} \sum_{k=0}^H e^{-\frac{(t + \frac{k}{H}dt - t_n)}{\tau_c}}}. \quad (32)$$

Until this step,  $\alpha$  is considered as a free parameter. However, it is obvious that the muscle will not be stimulated by whatever amplitude. In our case, we suppose that  $\alpha_i$  can range between 0 and 2, which corresponds to 2 times the stimulation constraint imposed in [2] (the pulse amplitude is still in an acceptable range).

## 4 Simulations Results

Differential equations of the force model (1) to (3) are solved by numerical methods. The control method is applied on the force model for the force references  $F_{ref} = 100, 200, 400, 600$  and 800 N with stimulation times  $dt = 10, 20, 40, 60, 80, 100$  ms.

In the Figures 1 and 3, the generated force for  $F_{ref} = 100, 200, 400, 600$  and 800 N is represented with the corresponding computed  $\alpha$  (Figures 2 and 4) (case of unconstrained  $\alpha$ ). The developed force staying constant at its final value during the simulation, we represent just the obtained force for a 1 s and 10 s duration. Contrary to the cases of small reference values (100, 200 and 400 N) where the impulse amplitude is at most equal to 0.2 (Figure 2), the  $\alpha$  values for  $F_{ref} = 600$  and 800 N reach very high values (Figure 4). As discussed above, the applied pulse to the muscle must have a reasonable amplitude. The effects of this constraint is showed in Figure 5 where  $\alpha$  is limited to 0.5, 1 and 2 for  $F_{ref} = 800$  N. It can be observed that  $\alpha$ 's limit influences the final value of  $F$ . In fact, the smaller  $\alpha$  is, the farther the final value of  $F$  is from  $F_{ref}$ .

In Figure 6, we treat the effect of  $dt$  ( $dt$  varies for 10, 20, 40, 60, 80 and 100 ms) on the final value of the force for  $F_{ref} = 100, 200, 400, 600$  and 800 N. It is clear that the difference between  $F$  and  $F_{ref}$  increases with  $dt$ .

To get closer to experimental results, a white noise of 5% seems adequate to mimic realistic conditions, that's why a 5% noise is added to the force measurements in all the control simulations. On the Figure 7, the obtained force is presented. At high reference force, the noise is not negligible and we must take into account the disturbance on the force and on the stimulation. With a low reference force, the developed force is not disturbed by noise.

## 5 Conclusion

In this work, we applied a control method to control the force value of a muscle during a stimulation session. The computed control method acts on the electrical impulse amplitude during an EMS. The simulation results showed a good efficiency of this control by maintaining the force at the reference force. Stimulation time and impulse amplitude effects were also explored for different cases of reference forces. A small stimulation time with a constrained impulse amplitude seems to be the best strategy to compute an efficient control. In a next study, it would be interesting to include muscular fatigue effects in order to check if this control could be still efficient then to test experimentally.

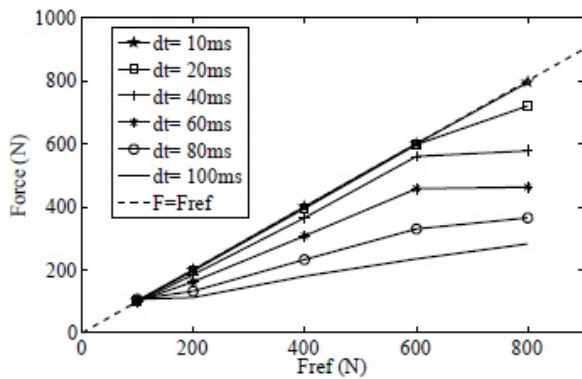


Figure 6: Application of the nonlinear control for the reference forces  $F_{ref}= 100, 200, 400, 600$  and  $800$  N, the obtained forces for  $dt= 10, 20, 40, 60, 80, 100$  ms.

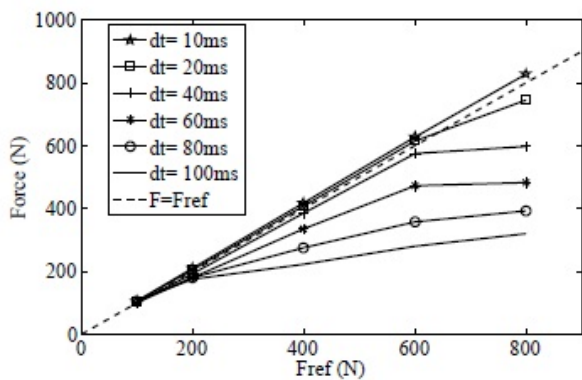


Figure 7: Application of the white noise of 5% for the  $F_{ref}= 100, 200, 400, 600$  and  $800$  N and  $dt= 10, 20, 40, 60, 80, 100$  ms.

**Acknowledgements:** The authors would like to thank the Conseil Regional de Bourgogne which supports the project through a young researcher contractor funding

#### References:

- [1] Z. Li, M. Hayashibe, C. Fattal and D. Guiraud, "Muscle fatigue tracking with evoked EMG via recurrent neural network: toward personalized neuroprosthetics", IEEE Computational Intelligence Magazine, 2014, 9 (2), 38-46.
- [2] J. Ding, A. S. Wexler and S. A. Binder-Macleod, "A predictive fatigue model-I: Predicting the effect of stimulation frequency and pattern on fatigue", IEEE Transactions on Neural Systems and Rehabilitation, vol 10, no 1 March 2002.
- [3] J. Ding, A. S. Wexler, and S. A. Binder-Macleod, "A predictive fatigue model-II: Predicting the ef-

fect of resting times on fatigue", IEEE Transactions on Neural Systems and Rehabilitation, vol 10, no 1 March 2002.

- [4] Li-Wei Chou, Jun Ding, Anthony S. Wexler, Stuart A. Binder-Macleod, "Predicting optimal electrical stimulation for repetitive human muscle activation", International Congress Series 15 (2005) 300-309.
- [5] Jun Ding, Stuart A. Binder-Macleod, Anthony S. Wexler, "Two-step, predictive, isometric force model tested on data from human and rat muscles", Journal of Applied Physiology 85 (1998) 2176-2189.
- [6] Jun Ding, Anthony S. Wexler, Stuart A. Binder-Macleod, "A mathematical model that predicts the force-frequency relationship of human skeletal muscle", Wiley Periodicals, Inc. Muscle Nerve 26 (2002) 477-485.
- [7] Samuel C. K. Lee, Jun Ding, Laura A. Prosser, Anthony S. Wexler, Stuart A. Binder-Macleod, "A predictive mathematical model of muscle forces for children with cerebral palsy", Developmental Medicine and Child Neurology, 2009, 51: 949-958.